

Sample Enhanced Visual Inspection of medical devices

SUBJECT: Enhanced Visual Inspection of medical devices

DEPARTMENT: Sterile Processing Area**

APPROVED BY:

EFFECTIVE:

REVISED: 9/2017

PURPOSE: The purpose of this policy is to provide a means of inspecting the cleanliness of medical devices with enhanced visual inspection (magnification, flexible inspection scopes, cameras...) as part of a departmental quality improvement process to ensure that all medical devices are clean and functional and can proceed to their next step in their reprocessing cycle.

POLICY: The Sterile Processing manager (or their designee) shall be responsible for selecting the type of medical devices and the frequency of the monitoring of those medical devices by enhanced visual inspection.

RATIONALE:

Visual clean is and always will be the standard. Every sterile processing professional knows if a medical device is dirty they must send the medical device back to be cleaned properly. A sterile processing professional must make sure all medical devices are clean and functional before they get sterilized or High Level Disinfected (HLD).

The process of using the unaided eye, alone or in conjunction with various aids (hand held magnifier, borescope, stain identification) to inspect medical devices for defects in functionality, pitting, stains, imperfections on the medical device during its processing cycle and rejecting the medical device according to the medical devices IFU if any of these imperfections are found is essential to providing a clean and functional medical device. Thus, the term enhanced visual inspection means using some form of magnification to enhance the visual inspection process.

“Make sure instrument surfaces are visibly clean and free from stains and tissue.”¹

“Instruments must be checked visually – tactile and be macroscopically clean (i.e. free from visible residues). This is checked by visual inspection. Critical area such as handle structures, joints or jaw serrations (particularly atraumatic

toothings) require especially careful checking. It is advisable to use working lights, such as light magnifying glasses with lenses of 3 to 6 diopters when checking filigree working ends".²

*"Cleaning encompasses the removal of patient secretions and excretions and of microorganisms from the patient or from handling or water exposure during reprocessing. After completing the cleaning process, personnel should visually inspect each item carefully to detect any visible soil. Inspection using magnification might identify residues more readily than the unaided eye"*³.


*"The most common method is a visual inspection, sometimes involving the use of a lighted magnifying glass. Health care personnel inspect every device for visible organic soil and contamination in a simple functionality check, usually as part of the inspection, preparation, and packaging procedure"*⁴.

All medical devices should be cleaned and inspected according to recommended standards and the manufacturers published Instructions for Use (IFU)^{5,6}. The visual inspection of the instruments provides a means of ensuring that each complex medical device can be routinely cleaned in the department. Many medical devices are difficult to inspect and are better viewed through the use of enhanced visual inspection like a flexible inspection scope or magnification devices. The department shall incorporate these tools to visually inspect both the external and internal surfaces and use such devices to ensure that the medical devices are visible clean and ready for the next step in the reprocessing cycle.

The term visual clean will be defined by referencing the IFU of the medical devices being inspected. This could be different for each medical device that is being inspected.

An example is the orthopedic shaver:

Shavers: Areas to inspect include the following:

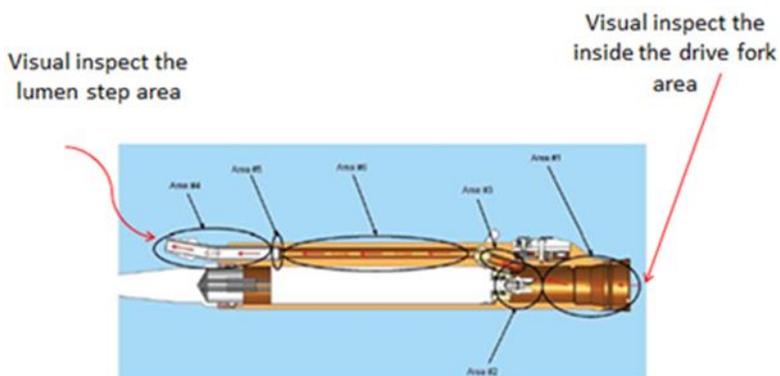

IFU Support for using a Flexible Inspection Scope:

1. Arthrex Hand Piece: The IFU states the following, “Check the device for visible soil. It is recommended that the cannulation be inspected with an illuminated, magnifying scopes. Clean the device using the guidelines for manual cleaning if any soil is visible...”.⁷

2. STRYKER Shaver Hand Piece: The IFU states the following, “Visually inspect the hand piece, including all internal surfaces, for remaining soil. Use an endoscopic camera and endoscope if necessary to see the inner surface of the lumen. If soil remains, repeat the manual cleaning procedure, focusing on those areas...”.⁸

In an FDA Safety Communication, “Consider inspecting the inside of the devices following cleaning to ensure that they have been cleared of any tissue or fluids. There may be multiple ways to accomplish this. As one example, the facility that brought this situation to our attention uses a 3mm video scope to inspect the channels of the shaver handpiece.”⁹

It is important to note that if using magnification, it should be documented or recorded in at least the count sheet record as a task performed to ensure the device is clean and functional.

PROCEDURE: The Sterile Processing manager (or their designee) is responsible for determining the type of medical devices to be visually inspected using some type of enhanced magnification, like a flexible inspection scope or other means according to that specific medical devices IFU. In cases where the manufacturer’s instructions for use state “inspection should be done under magnification”^{10, 11}, all such devices should be inspected in this manner every time they are reprocessed. Unclean or dirty medical devices pose a potential risk not only to patients but staff. Medical devices that are visibly dirty will be sent back to be re-cleaned according to the medical device manufactures IFU. All inspection results are recorded and in turn, this allows the Sterile Processing staff the ability to monitor and improve their cleaning process based on the data from their inspection (problem analysis).

In AAMI ST79 Visual inspection is described as a verification of the Cleaning process. Section 7.5.5 states the following:

- After completing the cleaning process, personnel should visually inspect each item carefully to detect any visible soil.
- Inspection using magnification might identify residues more readily than the unaided eye.
- Visual inspection alone may not be sufficient for assessing the efficacy of cleaning processes; the use of methods that are able to measure organic

residues that are not detectable using visual inspection should be considered in facility cleaning policy and procedures (see Annex D for available methods).

The manager of the Sterile Processing Area will determine when and the type of magnification (hand held, bench magnifier, borescope...) that should be used to inspect medical devices within their process.

"A problem analysis should be completed for any problem with any aspect of decontamination that can pose a risk to personnel or patients. The problem analysis should define and resolve the problem and the system should be monitored to ensure that the problem has been corrected."¹²


It is important to remember that documentation is important "if a process is not documented it was not performed...Jurors view good record keeping as an indicator of good care — poor documentation can create an aura of poor care and damage the credibility of the healthcare providers."¹³

An example of a log sheet to record enhanced visual inspection is included with this policy. This can also be accomplished if you have a computer system and this would be considered a task and must be checked off before going to the next task. Also, a reference flow chart on inspection is later in this sample policy.

RESPONSIBILITY: The Sterile Processing manager (or their designee) is responsible for assuring staff training, initiation, completion, documentation and analysis of the enhanced visual inspection policy for the department.

** According to ANSI/AAMI ST 79 the Sterile Processing Area is the area within a health care facility that processes and controls medical supplies, devices, and equipment, sterile and not sterile, for some or all patient care areas of the facility. This department is also known as the central service department, sterile processing, central processing and distribution and other names. Thus, for the purpose of this policy the Sterile Processing Area will be used to be consistent with ANSI/AAMI ST 79.

Site and Surface Inspection

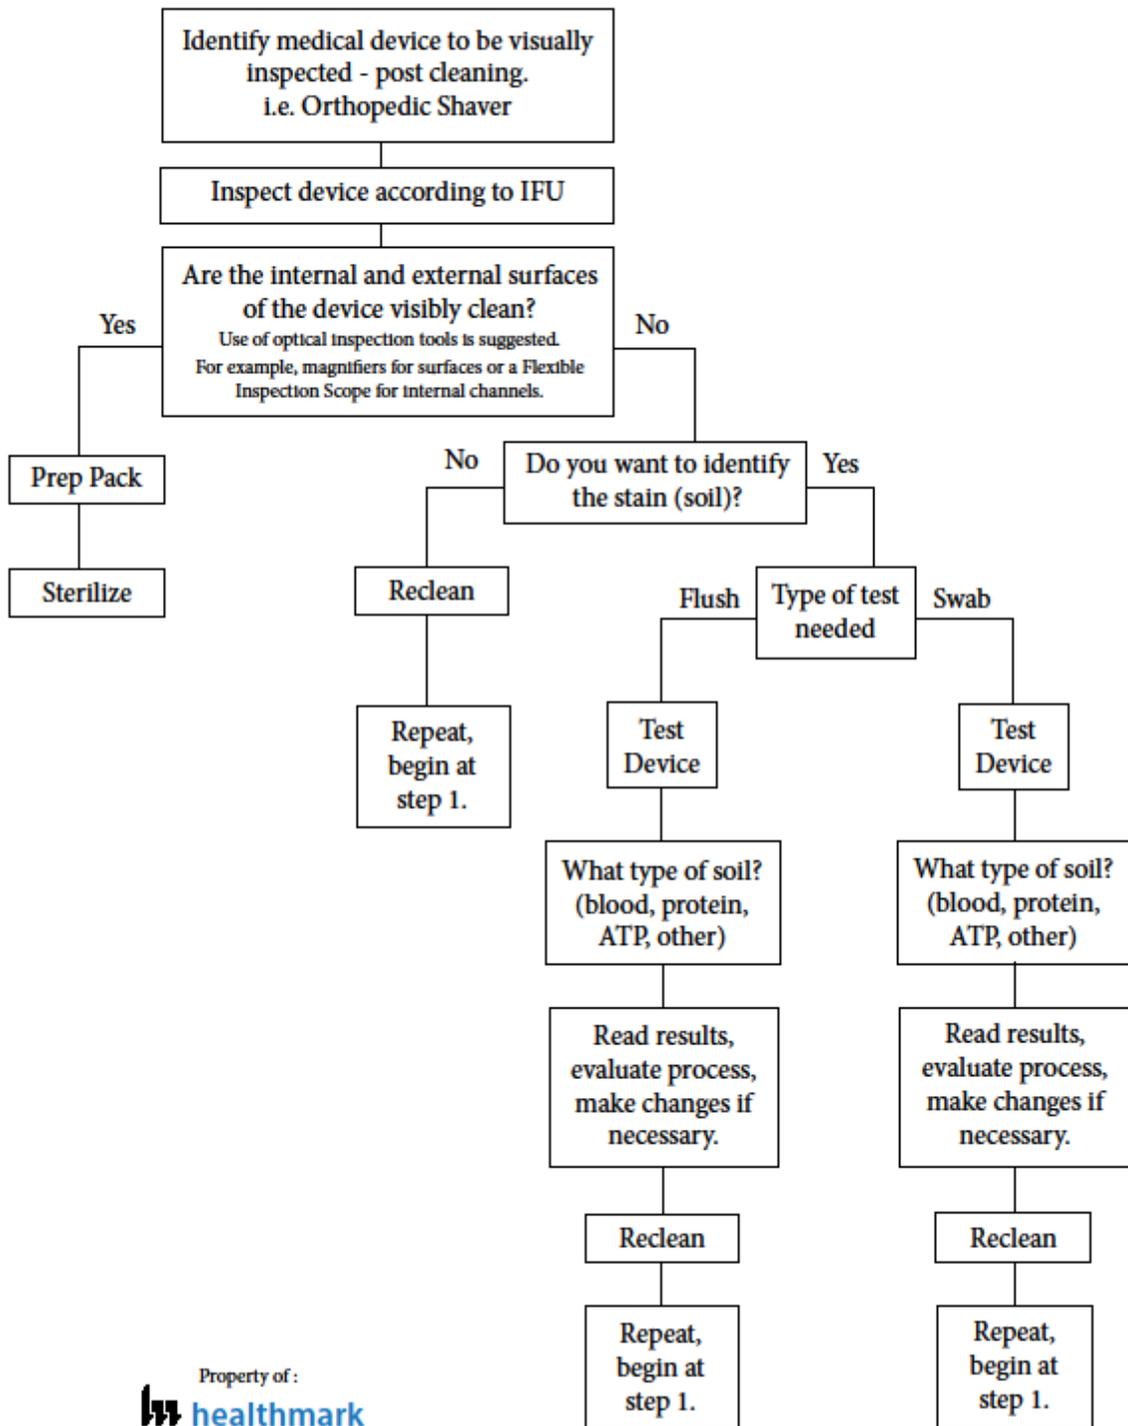

**Inspection Table
(Results of Visual Inspection)**

Date of Inspection	Inspector initials	Medical device tested/ make / model / serial number	Visual Clean* Yes / No	Comment
			Visual Clean Yes / No	
			Visual Clean Yes / No	
			Visual Clean Yes / No	
			Visual Clean Yes / No	
			Visual Clean Yes / No	

***If a medical device is found to be visually dirty (unclean) by inspection according to that specific medical device IFU, it must be sent back to be re-cleaned and then re-inspected until visually clean to proceed to the next step in its reprocessing cycle.**

Comments :

General Competency Record for the Visual Inspection of medical devices

Name: _____

Competency Statement: Complies with policy and procedure for ...list policy here
Key

1 = Performs independently and consistently. Ask for assistance in new situations.

2 = Performs with minimal guidance and direction. Asks for assistance when necessary.

3 = Performs with maximal guidance and direction. Preceptor dependent. Consistently needs assistance.

Comments:

Competency Achieved: _____(Date)

Evaluator: _____

Learner: _____

Because there are different methods / equipment that can be used to visually inspect medical devices this is a generic competency and the user must select the correct inspection device for that specific medical device that will need enhanced visual inspection. It is suggested in AAMI ST 79 that "Cleaning encompasses the removal of patient secretions and excretions and of microorganisms from the patient or from handling or water exposure during reprocessing. After completing the cleaning process, personnel should visually inspect each item carefully to detect any visible soil. Inspection using magnification might identify residues more readily than the unaided eye".

"The most common method is a visual inspection, sometimes involving the use of a lighted magnifying glass. Health care personnel inspect every device for visible organic soil and contamination in a simple functionality check, usually as part of the inspection, preparation, and packaging procedure".

Critical Behaviors	1	2	3
Review Hospital Policy on visual inspecting medical devices using the enhanced visual method of inspecting.			
Describes the purpose of visually inspecting medical devices.			
Gather appropriate supplies / equipment to perform the task of visually inspecting medical devices (flexible inspection scope, magnifying glass with illumination...).			
Read the specific instructions for use on the medical device you are going to inspect.			
First visually inspect the medial device with your natural eyesight and light. If the device is visually dirty, re-clean it according to its specific IFU.			
If the medical device states to use some enhanced form of inspection beyond the unaided eye like a bench style magnification product use it to inspect the medical device. If the device is found to be clean, follow the IFU for the next step in the process; if found dirty send back to be re-cleaned according to the IFU.			
If medical device is visually clean by natural eyesight and light and basic magnification, proceed to the form of enhanced visual inspection found in the IFU (example: orthopedic shaver suggests using some type of flexible inspection scope to look inside various parts of those devices to ensure it is visibly clean).			
If upon enhanced visual inspection the device is dirty, send it back to be re-cleaned. If it is deemed clean and not visually dirty send the device to the next step in its process.			
Document all results of the inspection on a log sheet / record book/ computer system. Sometimes this documentation entails the serial and model number of the device checked with enhanced visual inspection is recorded.			

Follow Hospital Policy on enhanced visual inspection of medical devices.

Remember to always follow manufactures guidelines (IFU) on inspecting medical devices.

Competency Record for using the Healthmark Flexible Inspection Scope

Name: _____

Competency Statement: Complies with policy and procedure for ...list policy here
Key

1 = Performs independently and consistently. Ask for assistance in new situations.

2 = Performs with minimal guidance and direction. Asks for assistance when necessary.

3 = Performs with maximal guidance and direction. Preceptor dependent. Consistently needs assistance.

Comments:

Competency Achieved: _____(Date)

Evaluator: _____

Learner: _____

This is a general competency that can be used for training staff on the proper use of the Healthmark Flexible Inspection Scope. This competency can be adjusted according to each facility specific requirement.

Critical Behaviors	1	2	3
Review Hospital Policy on visual inspecting medical devices using the Flexible Inspection Scope			
Describes the purpose of visually inspecting medical devices both with the unadded eye (in natural light) and with using the Flexible Inspection Scope			
Read / review the specific instructions for the Healthmark Flexible Inspection Scope			
Gather appropriate supplies / equipment to perform the task of visually inspecting medical devices with the Flexible Inspection Scope			
Selects appropriate devices for inspection with			

flexible inspection scope: instruments with cannulas or holes > or = in mm or larger in diameter the flexible inspection scope to ensure it will pass through easily according to policy.			
First visually inspect the medial device with your natural eyesight and light. If the device is visually dirty, re-clean it according to its specific IFU.			
If medical device is visually clean by natural eyesight and light proceed to the form of enhanced visual inspection found in the IFU (example: orthopedic shaver suggests using some type of flexible inspection scope to look inside various parts of those devices to ensure it is visibly clean).			
Before using the Flexible Inspection Scope on the medical device, you must demonstrate the following.			
Ensures scope is plugged in to a USB 2.0 plug before opening software.			
Ensure that the icon for the Flexible Inspection Scope short cut is on the computer screen			
Double clicks on Healthmark software icon to run program.			
The program will than recognize that a Flexible Inspection Scope is properly hooked up and you can than proceed.			
Demonstrates illumination feature, photo capture, record and review feature by clicking on software icons or scope buttons.			
Inserts scope tip into lumens or holes and demonstrates 100-degree view of lumen by maneuvering scope through lumen, avoiding any restrictive areas that may damage the scope tip.			
If upon enhanced visual inspection the device is dirty, send it back to be re-cleaned. If it is deemed clean and not visually dirty in the areas inspected send the device to the next step in its process.			
After each inspection, wipe down Flexible Inspections Scope with alcohol. Place the protective cap over the lens when not in use to protect the distal tip from damage			
Document all results of the inspection on a log sheet / record book. Sometimes this documentation entails the serial and model number of the device checked with a Flexible Inspection Scope. Follow your facilities policy on documentation.			

¹ Miltex Surgical Instruments Catalog; Clean, Sterilization & Maintenance of Surgical instruments section; 2005 Miltex

² AKI – Working Group Instrument Reprocessing; Red Book 10 Edition; Page 48

³ 2013 Association for the Advancement of Medical Instrumentation ■ ANSI/AAMI ST79:2010 & A1 & A2 & A3 & A4; 7.5.5 Verification of the cleaning process

⁴ 2013 Association for the Advancement of Medical Instrumentation ■ ANSI/AAMI ST79:2010 & A1 & A2 & A3 & A4; Annex D

⁵ STRYKER Shaver Hand Piece; 1000400638 R-2012/10; INSPECTION – EN 21; www.stryker.com

⁶ Arthrex - Adapter Power System™ II (APS II); Shaver Hand pieces -DFU-0154r10; www.arthrex.com

⁷ Arthrex Adapter Power System™ II (APS II) Shaver Hand pieces DFU-0154r10, Inspection and Maintenance Step 4. www.arthrex.com

⁸ STRYKER Shaver Hand Piece – 1000400638 R-2012/10 IFU, Inspection – EN21, Step 9. www.stryker.com

⁹ FDA Safety Communication. Ongoing Safety Review of Arthroscopic Shavers: FDA Safety Communication. 2015: Archived content. www.fda.gov

¹⁰ STRYKER Shaver Hand Piece; 1000400638 R-2012/10; INSPECTION – EN 21; www.stryker.com

¹¹ Arthrex - Adapter Power System™ II (APS II); Shaver Hand pieces -DFU-0154r10; www.arthrex.com

¹² 2013 Association for the Advancement of Medical Instrumentation ■ ANSI/AAMI ST79:2010 & A1 & A2 & A3 & A4; 11.2.3 Decontamination

¹³ <http://www.outpatientsurgery.net/surgical-facility-administration/avoid-medical-malpractice/how-to-survive-a-med-mal-suit--orx-proceedings-13?utm-source=tod&utm-medium=email&utm-campaign=tips>